

ACCEPTED MANUSCRIPT

Myotonometry as a measure to detect myofascial trigger points: an inter-rater reliability study

To cite this article before publication: Carolina Jiménez-Sánchez *et al* 2018 *Physiol. Meas.* in press <https://doi.org/10.1088/1361-6579/aae9aa>

Manuscript version: Accepted Manuscript

Accepted Manuscript is “the version of the article accepted for publication including all changes made as a result of the peer review process, and which may also include the addition to the article by IOP Publishing of a header, an article ID, a cover sheet and/or an ‘Accepted Manuscript’ watermark, but excluding any other editing, typesetting or other changes made by IOP Publishing and/or its licensors”

This Accepted Manuscript is © 2018 Institute of Physics and Engineering in Medicine.

During the embargo period (the 12 month period from the publication of the Version of Record of this article), the Accepted Manuscript is fully protected by copyright and cannot be reused or reposted elsewhere.

As the Version of Record of this article is going to be / has been published on a subscription basis, this Accepted Manuscript is available for reuse under a CC BY-NC-ND 3.0 licence after the 12 month embargo period.

After the embargo period, everyone is permitted to use copy and redistribute this article for non-commercial purposes only, provided that they adhere to all the terms of the licence <https://creativecommons.org/licenses/by-nc-nd/3.0>

Although reasonable endeavours have been taken to obtain all necessary permissions from third parties to include their copyrighted content within this article, their full citation and copyright line may not be present in this Accepted Manuscript version. Before using any content from this article, please refer to the Version of Record on IOPscience once published for full citation and copyright details, as permissions will likely be required. All third party content is fully copyright protected, unless specifically stated otherwise in the figure caption in the Version of Record.

View the [article online](#) for updates and enhancements.

1
2
3 **MYOTONOMETRY AS A MEASURE TO DETECT MYOFASCIAL TRIGGER**
4 **POINTS: AN INTER-RATER RELIABILITY STUDY**
5
6

7 **Authors**

8 Jiménez-Sánchez C¹, Ortiz-Lucas M¹, Bravo-Esteban E², Mayoral-del Moral O³, Herrero-Gállego P¹, Gómez-
9 Soriano J^{2,4}
10

11 **Affiliations**

12
13 ¹Iphysio Research Group, Universidad San Jorge, Zaragoza, Spain.

14
15 ²Toledo Physiotherapy Research Group (GIFTO). E.U.E. Fisioterapia de Toledo, Universidad Castilla La
16 Mancha. Toledo, Spain.

17
18 ³Physical Therapy Unit. Hospital Provincial. Toledo, Spain.

19
20 ⁴Sensorimotor Function Group, Hospital Nacional de Paraplégicos, Toledo, Spain.

21 **Corresponding author**

22
23 Name: María Ortiz-Lucas.

24
25 Mailing address: Facultad de Ciencias de la Salud, Universidad San Jorge, Campus Universitario Villanueva de
26 Gállego, Autov. A-23 Zaragoza-Huesca Km. 299, 50830 Villanueva de Gállego, Zaragoza, Spain

27
28 E-mail address: mortiz@usj.es

29
30 Telephone: (+34)976060100

31
32 Fax: (+34)976077581

33
34 **Word count:**

35
36 Abstract: 257

37
38 Manuscript: 4571
39
40
41
42
43
44
45
46
47
48
49
50
51
52
53
54
55
56
57
58
59
60

Abstract

Objective: Several diagnostic methods have been used in the identification of mechanical properties of skeletal muscle, including myofascial trigger points (MTrPs), but not suitable for daily clinical use. Myotonometry offers an easy noninvasive alternative to assess these muscle properties. Nevertheless, previous research has not yet studied the mechanical properties of MTrPs by myotonometry. The purposes were (1) to analyze differences in the mechanical properties between latent MTrPs and their taut bands by myotonometry, (2) to investigate the inter-rater reproducibility of myotonometric measurements and (3) to examine the association between myotonometry and passive isokinetic dynamometry. *Approach:* Fifty individuals (58% male; age 24.6 ± 7.9 years) with a latent medial MTrP of the right soleus muscle participated. Mechanical properties of this MTrP area of soleus muscle and its taut band area were measured using a myotonometer (MyotonPRO). Additionally, passive resistive torque and extensibility of triceps surae muscle was assessed using a Kin-Com dynamometer. *Main results:* Statistical analysis indicated higher values for stiffness parameter in the taut band with respect to MTrP ($P < 0.05$). The inter-rater reliability of the myotonometric measurements was good for all variables ($ICC_{3,1} > 0.75$). Standard error of measurement (SEM) and minimal detectable difference (MDD) indicated small measurement error for frequency and stiffness variables ($SEM\% < 10\%$; $MDD_{95}\% < 20\%$). Significant fair correlations between myotonometric parameters and passive isokinetic parameters were ranged from -0.29 to 0.48 ($P < 0.05$). *Significance:* The myotonometer was demonstrated to be a reliable tool and was able to quantify differences in the mechanical properties of myofascial tissues. The potential of this method for the assessment of myofascial pain syndromes requires further investigation.

Keywords: muscle stiffness, myofascial tissue, myotonometer, isokinetic dynamometer.

1. Introduction

Myofascial trigger points (MTrPs) are painful areas in skeletal muscle that are associated with a palpable nodule within a taut band of muscle fibers (Thomas and Shankar 2013, Simons 2014). These trigger points can exist in active or latent states. An active MTrP is characterized by spontaneous and/or mechanical local and/or referred pain, while a latent MTrP is a sensitive spot whose pain is only elicited in response to different kinds of stimulation, such as compression (Simons and Travell 1999). Nevertheless, the diagnosis of both types of MTrP is similar (Celik and Mutlu 2013).

Several methods have been employed over the years to measure the nature and characteristics of MTrP and taut bands. The usual diagnosis of a MTrP consists of the identification of a tender nodule within a taut band through palpation and the reproduction of the patient's symptoms in the case of active MTrPs (Simons 2008). However, this specific diagnosis depends on the experience, training and skills of the rater (Barbero *et al* 2013) and different inter-rater reliabilities have been reported (Barbero *et al* 2012, Gerwin *et al* 1997, Mayoral *et al* 2017; Sha and Heimur 2012). For that reason, today, the objective diagnosis and the quantification of its physical characteristics are crucial for improving treatment and clarifying the pathophysiology of MTrPs (Adigozali *et al* 2017).

Muscle stiffness and muscle tone are terms that have been often used interchangeably (Aarrestad *et al* 2004). Muscle tone can be defined as the resistance to passive stretch that reflects neural factors and mechanical or viscoelastic properties and is a term frequently used in the clinical context (Aarrestad *et al* 2004, Gómez-Soriano *et al* 2014, Masi and Hannon 2008). On the other hand, muscle stiffness includes active stiffness (considering reflex response and voluntary muscle contraction) and passive stiffness (mechanical or viscoelastic properties) and is a term more frequently used in biomechanics (Kubo 2014, Kubo *et al* 2015, Lorentzen *et al* 2010, Mirbagheri *et al* 2001). The impact of MTrPs development on muscle stiffness is still unknown.

More recently, new tools have been introduced to measure these muscle characteristics, such as magnetic resonance elastography, ultrasound elastography and tensiomyography. Magnetic resonance elastography and ultrasound elastography are musculoskeletal imaging modalities used to characterize skeletal muscle properties, such as tissue passive stiffness (Ballyns *et al* 2012, Basford and An 2009, Sikdar 2008, 2009, Simons 2008, Thomas and Shankar 2013, Turo *et al* 2015). However, these sophisticated techniques can cause deformations of the evaluated tissue and could alter the mechanical properties of muscle tissues depending on their basal state (Adigozali *et al* 2017, Viir *et al* 2006). Tensiomyography is also a noninvasive method to measure mechanical properties of superficial skeletal muscle, which has been used for the assessment of MTrP and the treatment effects (Calvo *et al* 2016, Calvo-Lobo *et al* 2017, Dahmane *et al* 2001). Although all these techniques provide objective measures of muscle stiffness characteristics, they are not suitable for clinical use, as they are expensive, time-consuming and require specialized staff training (Agyapong-Badu *et al* 2013).

Nevertheless, among these methods, the measurement of the resistance to passive stretch using an isokinetic dynamometry represents the gold standard assessment of muscle stiffness, being valid for assessing different muscle conditions (Boiteau *et al* 1995, Bressel and McNair 2002, Gomez Soriano *et al* 2014, Pisano *et al* 2000, Rabita *et al* 2005) but has never been employed in the evaluation of myofascial tissues stiffness.

Currently, the myotonometer, a simple, reliable, noninvasive, portable and painless tool, has already proven to be objective in measuring mechanical muscle properties. The myotonometer exerts a short mechanical pulse on the tested muscle, which causes a short-interval deformation in the muscle. The muscle responds to the mechanical stimulus in the form of damped oscillations recorded by an acceleration transducer on the testing end. After that, the device simultaneously computes biomechanical parameters of oscillation frequency, stiffness and logarithmic decrement (Chuang *et al* 2012, Lohr *et al* 2008). An important advantage is that the myotonometer setup, data acquisition and real-time results analysis requires considerably less time than other tools. Indeed, this method doesn't require considerable expertise and equipment and it is practical for daily clinical use (Fröhlich-Zwahlen *et al* 2014, Lo *et al* 2017, Van Deun *et al* 2014). Moreover, to our knowledge, no myotonometric study has reported the reliability and the assessment of MTrPs.

Therefore, the primary objective of this study was to determine the ability of the myotonometer to identify, quantify and compare the mechanical properties of the MTrP within its taut band, as well as to determine the inter-rater reliability of this measuring tool. As a secondary objective, the strength of the correlation between myotonometric and passive isokinetic parameters was established.

2. Methods

2.1. Design

1
2
3 The experimental design was a cross-sectional design conducted in accordance with The Declaration of
4 Helsinki. This study was approved by the Toledo Hospital Clinical Research Ethics Committee (protocol
5 number 134, 11/12/2015).

6
7 All participants completed a unique experimental session in which a myotonometry of a latent MTrP of the
8 soleus muscle and its taut band was performed independently by two raters. Furthermore, passive resistive
9 torque and soleus muscle extensibility was assessed by a third rater using an isokinetic dynamometer.

10 2.2. Participants

11
12 Healthy volunteers from the local community (accepted age range 18–55) with the presence of a latent medial
13 MTrP of the right soleus muscle were recruited to participate in this study. All participants provided signed
14 informed consent prior to the initiation of assessment procedures.

15
16 The exclusion criteria included: (1) any history of ipsilateral lower limb severe injury or intervention (e.g.
17 fracture, surgical intervention); (2) reported pain or musculoskeletal injury in the ipsilateral lower limb in the
18 previous month; (3) peripheral or central nervous system neurological disease; (4) altered sensitivity in the
19 studied area; and (5) treatment of a myofascial trigger point in the triceps surae muscle during the six months
20 previous to the study.

21 2.3. Procedures

22
23 All testing took place at the “Hospital Nacional de Paraplégicos” in Toledo (Spain) in a single session. A
24 specialized physiotherapist with more than 15 years of experience established the diagnosis of latent medial
25 MTrP of the right soleus muscle following the essential criteria proposed by Simons: focal spot muscle
26 tenderness and pressure-elicited referred pain pattern not recognized by the participant as a usual pain complaint
27 (Simons 2004, 2008). After that, this assessor located by manual palpation and marked on the skin the site of a
28 medial MTrP of soleus muscle and a selected point within its taut band, 1 cm distal to the marked medial MTrP.

29
30 Participants were seated in an isokinetic dynamometer (Kin-Com, Chattanooga Group Inc.) with the right hip
31 joint at 90° of flexion, the right knee slightly flexed at 10° and the right ankle in a neutral position on a footplate
32 aligned with the dynamometer rotation axis. The trunk and the right thigh were fixed with straps in order to
33 provide stability. A trained physiotherapist, rater 1, conducted the isokinetic dynamometer assessment.

34
35 Myotonometric measurements for inter-rater reliability were carried out by two different qualified raters, rater 2
36 and rater 3 within the same session, trained in the use of MyotonPRO technology.

37
38 In addition, another blinded researcher was responsible for entering outcome data on a data sheet.

39 2.4. Myotonometric Assessment

40
41 Participants were seated on the Kin-Com dynamometer and they were instructed to completely relax.
42 Myotonometric measures to compare the MTrP area and the taut band area were evaluated using the
43 MyotonPRO device (Müomeetria AS, Estonia). The myotonometer was held perpendicular and stable in the
44 measurement position. An automatically controlled preload (0.18 N) was applied with an automatic mechanical
45 impulse to the contact area, with a duration of 15 ms and a constant force of 0.4 N (Bailey *et al* 2013, Fröhlich-
46 Zwahlen *et al* 2014).

47
48 One measurement set of 10 consecutive impulses (scan mode) was completed at each of the two marked points
49 (the medial MTrP of the soleus muscle and its taut band) with a time interval of 1 s between each impulse. Mean
50 data of each series were accepted if the coefficient of variation of the measurement set was inferior to 3%
51 (Bailey *et al* 2013, Wang 2017). The parameters measured were: i) Oscillation frequency (Hz) as an indicator of
52 muscle tone, which characterizes the resting level of tension in the tissue; ii) logarithmic decrement [arbitrary
53 unit], which is considered as the ability of the muscle to restore its initial shape after being deformed (is
54 inversely proportional to elasticity); and iii) stiffness (N/m), which reflects the tissue resistance to the force
55 deforming the muscle (Aird *et al* 2012, Bailey *et al* 2013, Chuang *et al* 2013, Mullix *et al* 2012, Veldi *et al*
56 2000).

57 2.5. Passive Isokinetic Assessment

58
59 During all assessments, participants were asked to remain as relaxed as possible and instructed to press a panic
60 button to stop the assessment if it was necessary (Rabita *et al* 2005). Volunteers performed an initial warm-up

1
2
3 trial at each velocity to familiarize themselves with the Kin-com dynamometer (Chattanooga Group Inc.), which
4 consisted of 1 set of 5 passive mobilizations at slow velocity (10°/s) and 1 set of 10 passive mobilizations at fast
5 velocity (180°/s) (Boiteau *et al* 1995, Gomez-Soriano *et al* 2014, Rabita *et al* 2005). Then, the measurement of
6 muscle stiffness and muscle extensibility was performed.
7

8 Muscle stiffness was quantified by measuring the passive resistive torque of the triceps surae muscle when a
9 stretching was performed during the passive motion of the ankle joint from 35° plantar flexion to 5° dorsiflexion
10 at both velocities. The resistive force testing at slow velocity evidences the mechanical response to a muscle
11 stretch that does not evoke a reflex response. On the other hand, fast velocity represents total muscle stiffness,
12 including reflex-mediated resistance (Boiteau *et al* 1995, Gomez Soriano *et al* 2014, Lamontagne *et al* 1998,
13 Rydahl and Brouwer 2004). Peak torque (PT [Nm]) and average torque (AT [Nm]) during ankle dorsiflexion
14 were measured during both velocities as variables of the soleus muscle resistance (Gomez Soriano *et al* 2014).

15 The passive extensibility of skeletal muscles can be defined as the ability of a muscle to lengthen without
16 muscle activation, being the distance between an initial muscle length and the maximal length, both of which are
17 dependent on the passive resistance to the stretch (Gajdosik 2001, Weppler and Magnusson 2010). To evaluate
18 extensibility of the triceps surae muscle a passive range of motion (PRoM) at a constant velocity of 10°/s was
19 imposed from 35 degrees ankle joint plantarflexion to: (1) the maximum ankle dorsiflexion angle at which the
20 soleus muscle generated a resistance of 200 N (AA₂₀₀ [°]) (Gomez Soriano *et al* 2014), and (2) the ankle
21 dorsiflexion angle corresponding to the participant's perception endpoint of pain or stretch tolerance (AA_{Tol} [°])
22 (Weppler and Magnusson 2010).
23

24 2.6. Statistical analysis

25 Statistical analysis was performed using SPSS Version 21.0 (IBM Corporation, Armonk, NY) and the
26 SigmaPlot Version 11.0 (Systat Software, Canada).
27

28 The Shapiro–Wilk test was performed to determine normal data distribution. An independent Student t-test for
29 parametric data or Mann–Whitney U test for nonparametric data was performed to compare myotonometric
30 measurements performed at the medial MTrP with those obtained in the taut band of the soleus muscle.
31 Between-tissue effect sizes were calculated using Cohen's d coefficient. An effect size of less than 0.2 reflects a
32 negligible mean difference; between 0.2 and 0.5, a small difference; between 0.5 and 0.8, a moderate mean
33 difference; and 0.8 or greater, a large difference (Fritz *et al* 2012). To analyze correlations between the
34 myotonometric variables of the medial MTrP of the soleus muscle and the myotonometry variables of the taut
35 band, only the assessment made by rater 2 was selected.
36

37 Intra-class correlation coefficients (ICC_{3,1}) with 95% confidence interval (CI) were calculated to determine
38 relative reliability. An ICC of less than 0.50 was considered as poor reliability, 0.50 to 0.75 as moderate
39 reliability, and greater than 0.75 as good reliability (Portney and Watkins 2009). Absolute reliability indices
40 were expressed through standard error of measurement (SEM), SEM%, minimal detectable difference (MDD₉₅)
41 and MDD₉₅%. The SEM was estimated as the square root of the mean square error term from the analysis of
42 variance (ANOVA) (Hopkins 2000, Stratford and Goldsmith 1997, Weir 2005). The MDD at the 95%
43 confidence level was calculated using formula $MDD_{95} = SEM * (\sqrt{2}) * 1.96$ (Fleiss 2007, Portney and Watkins
44 2009). SEM and MDD values can be used to determine whether a change in a group or in an individual is
45 statistically significantly real (Chuang *et al* 2013). The smaller the SEM and the MDD, the greater the reliability
46 (Atkinson and Nevill 1998, Weir 2005). SEM% $(=SEM/mean \times 100)$, where mean is the mean for all
47 observations from both assessments and MDD₉₅% $(=(MDD_{95}/mean) \times 100)$, where mean is the mean for all
48 measurements from both assessments, were used to facilitate interpretation of the results (Flansbjerg *et al* 2005).
49 The SEM% of <10% can be considered small and makes it possible to detect small changes that indicate real
50 changes for a group of individuals (Chuang *et al* 2013, Flansbjerg *et al* 2005). The MDD₉₅% of below 30% can
51 be considered acceptable and that of below 10% can be considered excellent (Chuang *et al* 2013, Smidt *et al*
52 2002).
53

54 Pearson correlations (r) with 95% confidence interval (CI) were carried out to analyze the relationship between
55 myotonometric measurements of myofascial tissue and passive isokinetic parameters. The strength of
56 correlations was interpreted as low (0.00-0.25), fair (0.25-0.50), moderate to good (0.50-0.75) and good to
57 excellent (>0.75) (Portney and Watkins 2009).
58

59 Only the assessment made by rater 2 was selected for the correlation analysis with the isokinetic assessment
60 data.

All statistical analyses were performed considering a $P < 0.05$ significance level. Data are presented as mean \pm standard deviation.

3. Results

Fifty participants were recruited and completed full testing procedures. Characteristics of participants are described in Table 1.

3.1. Myotonometry of the Latent Myofascial Trigger Point and its Taut Band

The student t-test showed statistically significant differences for stiffness parameter ($P < 0.05$) when comparing the medial MTrP area of the soleus muscle with its taut band area for the assessment of both raters. Differences in stiffness for rater 2 and rater 3 were 23.7 N/m and 23.4 N/m, respectively, finding higher values in the taut band compared to MTrP for both assessments. No significant differences in frequency and decrement were observed in any assessment.

The mean (SD and CIs) myotonometric variables of the medial MTrP as well as myotonometric variables of the taut band are plotted in Table 2. Furthermore, Table 2 shows P values and effect sizes on myofascial tissues comparison, where MTrP showed a lower stiffness when compared with the taut band with $P < 0.05$ and effect size of $d = 0.465$ and $d = 0.431$ for rater 2 and rater 3 respectively.

3.2. Inter-rater Myotonometry Reliability

Table 3 shows ICCs and CIs, SEM (SEM%) and MDD_{95} ($MDD_{95}\%$) for the latent soleus medial MTrP and its taut band. A good general relative reliability ($ICC > 0.75$) was found for both MTrP and taut band measures, with a total range of 0.86 to 0.97. The SEM ranged from 0.35 to 0.63 Hz for frequency, from 0.17 to 0.24 for decrement and from 11.95 to 13.01 N/m for stiffness. The MDD_{95} was from 0.97 to 1.74 Hz for frequency, 0.48 to 0.68 for decrement and 33.12 to 36.07 N/m for stiffness. All the SEM% values were below 10% except for decrement parameter. In addition, the $MDD_{95}\%$ values for frequency and stiffness variables were below 12%, indicating a good absolute reliability. However this reliability result was not for decrement variable, obtaining values greater than 40%. In Figure 1, spaghetti graphs show data for all myotonometric variables, where each line connects values for both rater's measurements.

3.3. Association between Myotonometry Parameters within MTrP and Taut Band

Pearson correlation coefficient analysis among myotonometric variables of the medial MTrP of the soleus muscle and the taut band are shown in Table 4. There were general positive correlations for frequency, decrement and stiffness between the medial MTrP and its taut band.

3.4. Association between Myotonometry and Passive Isokinetic Dynamometry

Pearson r values between the myotonometric measurement variables and the passive isokinetic measurement variables are presented in Table 5. Correlations between frequency and stiffness myotonometric parameters of the medial MTrP and the taut band with respect to passive resistive torque to ankle dorsiflexion at $10^\circ/s$ and $180^\circ/s$ were fair and statistically significant with a range from 0.33 to 0.48 ($P < 0.05$). Decrement parameters of the medial MTrP and the taut band were negatively correlated with passive resistive torque to ankle dorsiflexion at $10^\circ/s$ ($r = -0.29$ to -0.31 , $P < 0.05$) and positively correlated with ankle dorsiflexion tolerance angle ($r = 0.33$, $P < 0.05$).

4. Discussion

This is the first study that measures the MTrP area and its taut band area using a myotonometer device and the data support that not only could myotonometry be useful to understand mechanical properties of the myofascial tissue, but it could also be useful for the diagnosis and detection of MTrP. The results of the present study showed that (1) myotonometry is able to distinguish between the viscoelastic properties of a latent MTrP and its taut band, (2) myotonometry is a reliable technique for the assessment of the myofascial tissue and (3) passive resistive torque of the triceps surae muscle measured with the isokinetic device positively correlates with the "frequency" and "stiffness" and negatively with "decrement" as measured by the myotonometer.

4.1. Specific Mechanical Properties of the Myofascial Trigger Points

This study supports the ability of the myotonometer device to identify and detect differences between the mechanical properties of the MTrP and their surrounding myofascial muscle tissue (taut band).

Interestingly, we found lower values of stiffness in latent soleus medial MTrP compared to its taut band in both raters' assessments. The higher the stiffness value, the more energy needed to modify the shape of the tissue. As expected, an excellent association between myotonometric variables of MTrP and taut band existed, considering we were evaluating points within the same myofascial structure in the soleus muscle.

Comparison of all these results with the literature is not possible because there are no reports on the myotonometric measurement of myofascial tissue. However, several studies have employed the myotonometer to quantify and distinguish other different muscle conditions (Chuang *et al* 2012, Fröhlich-Zwahlen *et al* 2014, Li *et al* 2017, Marusiak *et al* 2010, Van Deun *et al* 2017, Wang 2017). For example, previous studies focusing on the assessment of relaxed, contraction and stretching muscle states established differences in evaluated myotonometric parameters in these different muscle conditions (Alamaki *et al* 2007, Ditroilo *et al* 2011, Gavronski *et al* 2007, Ikezoe *et al* 2012). Higher values of frequency, stiffness and elasticity (inversely proportional to the decrement) in the contracted and stretched muscles with respect to the relaxed state were reported. Older adults present greater stiffness and frequency and lower elasticity than younger adults (Agyapong-Badu *et al* 2015). Findings from studies addressing muscle tone disorders show higher stiffness in the myotonometric measurement of skeletal muscle in Parkinson's patients with increased rigidity measured clinically (Marusiak *et al* 2010, Rätsep and Asser 2011) and in people with spasticity compared to healthy controls (Rydahl and Brouwer 2004). Similarly, myotonometric parameters differ depending on the position. According to Vain *et al* (2014) frequency and stiffness characteristics of the medial gastrocnemius muscle were significantly higher in the standing position compared to the supine position. Despite all these changes observed and the good reliability evidenced (Aird *et al* 2012, Bizzini and Mannion 2003, Chuang *et al* 2012, Marusiak *et al* 2010, Zinder and Padua 2011), we should have in mind that some authors are critical of this method (Pamukoff *et al* 2016, Rihvk *et al* 2010).

Several methods, such as electromyography, biochemical analysis, tensiomyography or elasticity imaging techniques (i.e. magnetic resonance elastography and ultrasound elastography) have been previously proposed in the literature to identify the presence and the type (active or latent) of MTrPs and to determine their tissue characteristics. A microanalytic and biochemical analysis showed higher concentrations for all analytes and lower pH in active MTrP than latent and absent MTrP in the upper trapezius muscle (Sha *et al* 2005). Furthermore, preliminary results of a nonpublished pathophysiological study show that MTrPs seem to present a higher content of glycosaminoglycans (GAGs) (Santafe *et al* 2015). This research about the composition of MTrPs could explain our findings of lower values of stiffness in the MTrP when compared with the surrounding area (taut band).

In this way, using ultrasound vibration sonoelastography, Sikdar *et al* (2008) found that there were differences in the echogenicity and echotexture of the MTrPs related to an increased stiffness both in active and latent MTrPs compared to normal tissue. Furthermore, magnetic resonance elastography studies in myofascial syndrome revealed that taut bands are indeed stiffer than the surrounding muscle in which they are found (Chen *et al* 2007, 2008, 2016). Another study showed the utility of ultrasound imaging to facilitate the detection of the taut band compared to the adjacent normal muscle tissue (Shankar and Reddy 2012). In addition, a recent study compared the use of sonoelastography and tensiomyography to detect stiffness differences among active MTrPs, latent MTrPs and control points, concluding that only sonoelastographic strain index could detect higher values of stiffness at the area of active and latent MTrPs compared to control points (Calvo-Lobo *et al* 2017). Further studies will be required to focus on linking these findings with myotonometric analysis in order to provide a better understanding of the mechanical properties of myofascial tissues.

4.2. Inter-rater Myotonometry Reliability

In reference to inter-rater reliability, ICCs were very high for all myotonometric outcomes. Moreover, for frequency and stiffness parameters, the SEM% values lay below 10% and MDD% values lay below 20%, which can be considered small and acceptable. The SEM (SEM%) and MDD₉₅ (MDD₉₅%) of the taut band assessment appear to be smaller than those of the MTrP assessment, indicating a more reliable measurement.

It is important to note that no study has evaluated inter-reliability in myofascial tissues before. Nevertheless, our reliability results are in concordance with previous studies using myotonometry in healthy subjects, where ICC scores were superior to 0.60 for frequency, decrement and stiffness parameters (Van Deun *et al* 2016, Viir *et al* 2006). In addition, Sakkool *et al* (2016) found in healthy children good inter-reliability for all measured muscles in their study, except for rectus femoris. Our results, except for decrement variable, regarding absolute reliability

are in line with other study's results where inter-reliability was studied in healthy subpopulations (Agyapong-Badu *et al* 2013; Van Deun *et al* 2017). However, Van Deun *et al* (2017) also found lower relative reliability in individuals with paratonia (Lohr *et al* 2008). Similar SEM% and MDD% values but in intra-rater reliability studies were found by Lohr *et al* (2018) and Van Deun *et al* (2017) in healthy adults and by Chuang *et al* (2013) in subacute stroke patients. It must be emphasized that these authors calculated absolute reliability through a different procedure using ICCs to obtain SEM values.

In scientific literature, myotonometric reproducibility between qualified physiotherapists and novice users was also evaluated. Agyapong-Badu *et al* (2013) demonstrated good and excellent inter-rater reliability in novice physiotherapists for the three myotonometric parameters in young and older healthy males. In an infantile cerebral palsy study, reliability in novice users was also studied in relaxed and contracted muscles, showing moderate to high results with some exceptions (Aarrestad *et al* 2004). According to these studies, myotonometric measurements provide objective data that are not influenced by the experience of the rater (Leonard *et al* 2003) in contrast to other MTrP assessments, such as manual palpation (Barbero *et al* 2012), imaging techniques (Takla *et al* 2016) or tensiomyography (Tous-Fajardo *et al* 2010).

4.3. Myotonometry as a Measure of Muscle Tone

Passive resistive torque while stretching a muscle using an isokinetic device is considered as a gold standard to measure muscle stiffness and quantify muscle tone disorders (Lamontagne *et al* 1998, Rabita *et al* 2005). On the other hand, myotonometry provides the assessment by quantifying tissue displacement with respect to perpendicular compression force. However, very few studies have compared myotonometric measurements with "the resistance to passive movement" paradigm (Leonard *et al* 2001, Li *et al* 2017, Rydahl and Brouwer 2004). Li *et al* (2017) reported similar correlation coefficients to our study between the total stiffness at 100°/s controlled by a servomotor and the degree of muscle deformation with respect to the compression applied perpendicularly to the muscle measured with another myotonometer device. Our significant but "low to moderate" correlations could be due to the different concept of muscle stiffness assessment. In the case of myotonometry, muscle stiffness is measured by the resistance of a perpendicular force to a determined point (Agyapong-Badu *et al* 2013, 2016). On the other hand, muscle stiffness quantified by isokinetic dynamometry is obtained by a longitudinally applied force to all the muscle-tendon and articular structures (Bressel and McNair 2002).

Other studies have revealed the relationship between myotonometry and other muscle stiffness assessment tools. Ditroilo *et al* (2011) studied the influence of the position of the knee joint on contractile and mechanical properties of the biceps femoris muscle by myotonometry and tensiomyography, concluding myotonometry presents higher sensitivity to detecting changes in the three myotonometric parameters (frequency, decrement and stiffness). Nevertheless, no correlations between these methods were realized in this study. In another study where muscle stiffness in Parkinson's disease patients was evaluated, myotonometric parameters have been shown to correlate with electromyographic recordings in the biceps brachii muscle. So, it is proposed that myotonometry could be an alternative method to assess muscle passive stiffness of skeletal muscle (Marusiak *et al* 2012).

Further research in both myotonometric assessment as well as isokinetic assessment is needed, taking into account latent and active MTrPs in different muscles.

4.4. Limitations

These results should be interpreted with caution since it should be emphasized that our study was carried out in latent MTrPs of asymptomatic adults. Future studies might focus on studying mechanical properties of active MTrPs in persons with myofascial pain syndrome. Another relevant point is that a control point outside the taut band of the muscle was not included in this study. The comparison of the MTrP and its taut band with a non-myofascial point would increase the understanding of myofascial tissue properties since the comparison of these structures has not yet been studied in scientific literature. Furthermore, the application of the myotonometry method on more superficial or deeper muscles should be considered, taking into account the body mass index. We haven't assessed intra-rater reliability but numerous myotonometric studies have showed a moderate to good intra-rater reliability within session (Chuang *et al* 2012, Lidström *et al* 2009, Lohr *et al* 2018) and between sessions (Aird *et al* 2012, Bizzini and Mannion 2003, Lohr *et al* 2018). The absence of myoelectric activities of triceps surae muscle has not been confirmed by electromyography and this is another acknowledged limitation. Finally, to enhance the applicability and interpretability of the myotonometric measurements, further studies are required to provide validity and reference values to examine potential applications of the MyotonPRO device in the diagnosis of and regular clinical practice in myofascial syndrome.

5. Conclusion

Our findings suggest that myotonometry is a reliable method to measure latent MTrPs and is able to detect differences in their physical characteristics with respect to taut bands. In addition, the moderate but significant correlation observed between myotonometry and the resistive torque measured by dynamometry suggests that myotonometry could be an easy and cheap tool for measuring muscle stiffness. However, it is necessary to establish whether both techniques assess the same stiffness characteristics of the muscle tissues.

References

- Aarrestad DD, Williams MD, Fehrer SC, Mikhailenok E, Leonard CT 2004 Intra- and interrater reliabilities of the Myotonometer when assessing the spastic condition of children with cerebral palsy *J Child Neurol.* 19(11):894-901 <http://dx.doi.org/10.1177/08830738040190110801>
- Adigozali H, Shadmehr A, Ebrahimi E, Rezasoltani A, Naderi F 2017 Reliability of assessment of upper trapezius morphology, its mechanical properties and blood flow in female patients with myofascial pain syndrome using ultrasonography *J Bodyw Mov Ther.* 21(1):35-40 <http://dx.doi.org/10.1016/j.jbmt.2016.04.010>
- Agyapong-Badu S, Aird L, Bailey L, Mooney K, Mullix J, Warner M, Samuel D, Stokes M 2013 Interrater reliability of muscle tone, stiffness and elasticity measurements of rectus femoris and biceps brachii in healthy young and older males *Working Papers in the Health Sciences* 1(4):1-11
- Agyapong-Badu S, Warner M, Samuel D, Stokes M 2016 Measurement of ageing effects on muscle tone and mechanical properties of rectus femoris and biceps brachii in healthy males and females using a novel hand-held myometric device *Arch Gerontol Geriatr.* 62:59-67 <http://dx.doi.org/10.1016/j.archger.2015.09.011>
- Aird L, Samuel D, Stokes M 2012 Quadriceps muscle tone, elasticity and stiffness in older males: reliability and symmetry using the MyotonPRO *Arch Gerontol Geriatr.* 55(2):e31-9 <http://dx.doi.org/10.1016/j.archger.2012.03.005>
- Alamäki A, Häkkinen A, Mälkiä E, Ylinen J 2007 Muscle tone in different joint positions and at submaximal isometric torque levels *Physiol Meas.* 28(8):793-802
- Atkinson G, Nevill AM 1998 Statistical methods for assessing measurement error (reliability) in variables relevant to sports medicine *Sports Med.* 26:217-38.
- Bailey L, Samuel D, Warner M, Stokes M 2013 Parameters representing muscle tone, elasticity and stiffness of biceps brachii in healthy older males: symmetry and within-session reliability using the MyotonPRO *J Neurol Disord.* 1:116
- Ballyns JJ, Turo D, Otto P, Shah JP, Hammond J, Gebreab T, Gerber LH, Sikdar S 2012 Office-based elastographic technique for quantifying mechanical properties of skeletal muscle *J Ultrasound Med.* 31(8):1209-19
- Barbero M, Bertoli P, Cescon C, Macmillan F, Coutts F, Gatti R 2012 Intra-rater reliability of an experienced physiotherapist in locating myofascial trigger points in upper trapezius muscle *J Man Manip Ther.* 20(4):171-7 <http://dx.doi.org/10.1179/2042618612Y.0000000010>
- Barbero M, Cescon C, Tettamanti A, Leggero V, Macmillan F, Coutts F, Gatti R 2013 Myofascial trigger points and innervation zone locations in upper trapezius muscles *BMC Musculoskelet Disord.* 14:179 <http://dx.doi.org/10.1186/1471-2474-14-179>
- Basford JR, An KN 2009 New techniques for the quantification of fibromyalgia and myofascial pain *Curr Pain Headache Rep.* 13(5):376-8
- Bizzini M, Mannion AF 2003 Reliability of a new, hand-held device for assessing skeletal muscle stiffness *Clin Biomech.* 18:459-461
- Boiteau M, Malouin F, Richards CL 1995 Use of a hand-held dynamometer and a Kin-Com dynamometer for evaluating spastic hypertonia in children: a reliability study *Phys Ther.* 75(9):796-802

- 1
2
3 Bressel E, McNair PJ 2002 The effect of prolonged static and cyclic stretching on ankle joint stiffness, torque
4 relaxation, and gait in people with stroke *Phys Ther.* 82(9):880-7
5
- 6 Calvo S, Quintero I, Herrero P 2016 Effects of dry needling (DNHS technique) on the contractile properties of
7 spastic muscles in a patient with stroke: a case report *Int J Rehabil Res.* 39(4):372-376
8
- 9 Calvo-Lobo C, Diez-Vega I, Martínez-Pascual B, Fernández-Martínez S, de la Cueva-Reguera M, Garrosa-
10 Martín G, Rodríguez-Sanz D 2017 Tensiomyography, sonoelastography, and mechanosensitivity differences
11 between active, latent, and control low back myofascial trigger points: A cross-sectional study *Medicine*
12 (Baltimore) 96(10):e6287 <http://dx.doi.org/10.1097/MD.00000000000006287>
- 13 Celik D, Mutlu EK 2013 Clinical implication of latent myofascial trigger point *Curr Pain Headache Rep.*
14 17(8):353 <http://dx.doi.org/10.1007/s11916-013-0353-8>
15
- 16 Chen Q, Basford J, An KN 2008 Ability of magnetic resonance elastography to assess taut bands *Clin Biomech.*
17 23(5):623-9 <http://dx.doi.org/10.1016/j.clinbiomech.2007.12.002>
18
- 19 Chen Q, Bensamoun S, Basford JR, Thompson JM, An KN 2007 Identification and quantification of myofascial
20 taut bands with magnetic resonance elastography *Arch Phys Med Rehabil.* 88(12):1658-61
21
- 22 Chen Q, Wang HJ, Gay RE, Thompson JM, Manduca A, An KN, Ehman RE, Basford JR(2016 Quantification
23 of Myofascial Taut Bands *Arch Phys Med Rehabil.* 97(1):67-73 <http://dx.doi.org/10.1016/j.apmr.2015.09.019>
24
- 25 Chuang LL, Lin KC, Wu CY, Chang CW, Chen HC, Yin HP, Wang L 2013 Relative and absolute reliabilities
26 of the myotonometric measurements of hemiparetic arms in patients with stroke *Arch Phys Med Rehabil.*
27 94(3):459-66 <http://dx.doi.org/10.1016/j.apmr.2012.08.212>
- 28 Chuang LL, Wu CY, Lin KC, Lur SY 2012 Quantitative mechanical properties of the relaxed biceps and triceps
29 brachii muscles in patients with subacute stroke: a reliability study of the myoton-3 myometer *Stroke Res Treat.*
30 617694 <http://dx.doi.org/10.1016/j.apmr.2015.09.019>
31
- 32 Dahmane R, Valen i V, Knez N, Er en I 2001 Evaluation of the ability to make non-invasive estimation of
33 muscle contractile properties on the basis of the muscle belly response *Med Biol Eng Comput.* 39(1):51-5
34
- 35 Ditroilo M, Hunter AM, Haslam S, De Vito G 2011 The effectiveness of two novel techniques in establishing
36 the mechanical and contractile responses of biceps femoris *Physiol Meas.* 32(8):1315-26.
37 <http://dx.doi.org/10.1088/0967-3334/32/8/020>
- 38 Flansbjerg UB, Holmback AM, Downham D, Patten C, Lexell J 2005 Reliability of gait performance tests in men
39 and women with hemiparesis after stroke *J Rehabil Med.* 37:75-82
40
- 41 Fleiss J 2007 Design and analysis of clinical experiments (New York: Wiley and Sons)
42
- 43 Fritz CO, Morris PE, Richler JJ 2012 Effect size estimates: current use, calculations, and interpretation *J Exp*
44 *Psychol.* 141(1):2-18 <http://dx.doi.org/10.1037/a0024338>
- 45 Fröhlich-Zwahlen AK, Casartelli NC, Item-Glatthorn JF, Maffioletti NA 2014 Validity of resting
46 myotonometric assessment of lower extremity muscles in chronic stroke patients with limited hypertonia: a
47 preliminary study *J Electromyogr Kinesiol.* 24(5):762-9 <http://dx.doi.org/10.1016/j.jelekin.2014.06.007>
48
- 49 Hopkins WG 2000 Measures of reliability in sports medicine and science *Sports Med.* 30:375-381
50
- 51 Gajdosik RL 2001 Passive extensibility of skeletal muscle: review of the literature with clinical implications
52 *Clin Biomech.* 16(2):87-101
53
- 54 Gavronski G, Veraksits A, Vasar E, Maaros J 2007 Evaluation of viscoelastic parameters of the skeletal
55 muscles in junior triathletes *Physiol Meas.* 28(6):625-37
56
- 57 Gerwin RD, Shannon S, Hong CZ, Hubbard D, Gevirtz R 1997 Interrater reliability in myofascial trigger point
58 examination *Pain* 69(1-2):65-73
59
60

- 1
2
3 Gómez-Soriano J, Abián-Vicén J, Aparicio-García C, Ruiz-Lázaro P, Simón-Martínez C, Bravo-Esteban E,
4 Fernández-Rodríguez JM 2014 The effects of kinesio taping on muscle tone in healthy subjects: a double-blind,
5 placebo-controlled crossover trial *Man Ther.* 19(2):131-6
6
- 7 Ikezoe T, Asakawa Y, Fukumoto Y, Tsukagoshi R, Ichihashi N 2012 Associations of muscle stiffness and
8 thickness with muscle strength and muscle power in elderly women *Geriatr Gerontol Int.* 12:86-92
9 <http://dx.doi.org/10.1111/j.1447-0594.2011.00735.x>
- 10 Kubo K 2014 Active muscle stiffness in the human medial gastrocnemius muscle in vivo *J Appl Physiol.* 117:
11 1020–1026 <http://dx.doi.org/10.1152/jappphysiol.00510.2014>
- 12
13 Kubo K, Miyazaki D, Yamada K, Yata H, Shimoju S, Tsunoda N 2015 Passive and active muscle stiffness in
14 plantar flexors of long distance runners *J Biomech.* 16;48(10):1937-43
15 <http://doi.org/10.1016/j.jbiomech.2015.04.012>
- 16
17 Lamontagne A, Malouin F, Richards CL, Dumas F 1998 Evaluation of reflex- and nonreflex-induced muscle
18 resistance to stretch in adults with spinal cord injury using hand-held and isokinetic dynamometry *Phys Ther.*
19 78(9):964-75
- 20
21 Leonard CT, Deshner WP, Romo JW, Suoja ES, Fehrer SC, Mikhailenok EL 2003 Myotonometer intra- and
22 interrater reliabilities *Arch Phys Med Rehabil.* 84(6):928-32
- 23
24 Leonard CT, Stephens JU, Stroppel SL 2001 Assessing the spastic condition of individuals with upper
25 motoneuron involvement: validity of the myotonometer *Arch Phys Med Rehabil.* 82:1416–1420
26 <http://dx.doi.org/10.1053/apmr.2001.26070>
- 27
28 Li X, Shin H, Li S, Zhou 2017 Assessing muscle spasticity with Myotometric and passive stretch
29 measurements: validity of the Myotonometer *Sci Rep.* 7:44022 <http://dx.doi.org/10.1038/srep44022>
- 30
31 Lidström A, Ahlsten G, Hirschfeld H, Norrlin S 2009 Intrarater and interrater reliability of Myotonometer
32 measurements of muscle tone in children *J Child Neurol.* 24(3):267-74
33 <http://dx.doi.org/10.1177/0883073808323025>
- 34
35 Lo WLA, Zhao JL, Chen L, Lei D, Huang DF, Tong KF 2017 Between-days intra-rater reliability with a hand
36 held myotonometer to quantify muscle tone in the acute stroke population *Sci Rep.* 7(1):14173
37 <http://dx.doi.org/10.1038/s41598-017-14107-3>
- 38
39 Lohr C, Braumann KM, Reer R, Schroeder J, Schmidt T 2018 Reliability of tensiomyography and
40 myotometry in detecting mechanical and contractile characteristics of the lumbar erector spinae in healthy
41 volunteers *Eur J Appl Physiol.* 118(7):1349-1359 <http://dx.doi.org/10.1007/s00421-018-3867-2>
- 42
43 Lorentzen J, Grey MJ, Crone C, Mazevet D, Biering-Sorensen F, Nielsen JB 2010 Distinguishing active from
44 passive components of ankle plantar flexor stiffness in stroke, spinal cord injury and multiple sclerosis *Clin
45 Neurophysiol.* 121(11):1939-51 <http://dx.doi.org/10.1016/j.clinph.2010.02.167>
- 46
47 Marusiak J, Kisiel-Sajewicz K, Jaskólska A, Jaskólski A 2010 Higher muscle passive stiffness in Parkinson's
48 disease patients than in controls measured by myotometry *Arch Phys Med Rehabil.* 91(5):800-2
49 <http://dx.doi.org/10.1016/j.apmr.2010.01.012>
- 50
51 Masi AT, Hannon JC 2008 Human resting muscle tone (HRMT): narrative introduction and modern concepts *J
52 Bodyw Mov Ther.* 12(4):320-32 <http://dx.doi.org/10.1016/j.jbmt.2008.05.007>
- 53
54 Mayoral Del Moral O, Torres Lacomba M, Russell IJ, Sánchez Méndez O, Sánchez Sánchez B 2017 Validity
55 and reliability of clinical examination in the diagnosis of myofascial pain syndrome and myofascial trigger
56 points in upper quarter muscles *Pain Med.* 00:1-12 <http://dx.doi.org/10.1093/pm/pnx315>
- 57
58 Mirbagheri MM, Barbeau H, Ladouceur M, Kearney RE 2001 Intrinsic and reflex stiffness in normal and
59 spastic, spinal cord injured subjects *Exp Brain Res.* 141(4):446-59
- 60
61 Mullix J, Warner M, Stokes M 2012 Testing muscle tone and mechanical properties of rectus femoris and biceps
62 femoris using a novel hand held MyotonPRO device: relative ratios and reliability *Working Papers in the Health
63 Sciences* 1(1):1-8

- 1
2
3 Pamukoff DN, Bell SE, Ryan ED, Blackburn JT 2016 The myotonometer: not a valid measurement tool for
4 active hamstring musculotendinous stiffness *J Sport Rehabil.* 25(2):111-6 [http://dx.doi.org/10.1123/jsr.2014-](http://dx.doi.org/10.1123/jsr.2014-0271)
5 [0271](http://dx.doi.org/10.1123/jsr.2014-0271)
6
7 Pisano F, Miscio G, Del Conte C, Pianca D, Candeloro E, Colombo R 2000 Quantitative measures of spasticity
8 in post-stroke patients *Clin Neurophysiol.* 111(6):1015-22
9
10 Portney LG, Watkins MP 2009 *Foundations of Clinical Research: Applications to Practice* 3rd edn Upper
11 Saddle River (New York: Prentice Hall Health)
12
13 Rabita G, Dupont L, Thevenon A, Lensele-Corbeil G, Pérot C, Vanvelcenaher J 2005 Quantitative assessment of
14 the velocity-dependent increase in resistance to passive stretch in spastic plantarflexors *Clin Biomech.*
15 20(7):745-53
16
17 Rätsep T, Asser T 2011 Changes in viscoelastic properties of skeletal muscles induced by subthalamic
18 stimulation in patients with Parkinson's disease *Clin Biomech.* 26(2):213-7
19 <http://dx.doi.org/10.1016/j.clinbiomech.2010.09.014>
20
21 Rihvk I, Clough A, Clough P 2010 Investigation to compare static stretching and proprioceptive neuromuscular
22 facilitation contract-relax stretching effects on the viscoelastic parameters of the biceps femoris muscle
23 *International Musculoskeletal Medicine* 32(4): 157-162
24
25 Rydahl SJ, Brouwer BJ 2004 Ankle stiffness and tissue compliance in stroke survivors: a validation of
26 Myotonometer measurements *Arch Phys Med Rehabil.* 85(10):1631-7
27
28 Sakkool T, Meerits T, Gapeyeva H 2016 Intrarater and interrater reliability of muscle tone, elasticity and
29 stiffness characteristics measurements by myoton-3 in healthy children aged 5-7 years *Baltic journal of sport &*
30 *health sciences* 1(100):38-46
31
32 Santafe Martinez, M, Margalef Perez R, Sisquella Basagaña M, Bosque Alberich M, Romeu Escolá C, Mayoral
33 del Moral O, Monterde Perez S, Priego Luque M, Ortiz Castellon N, Tomás Ferrer J 2015 Patophysiological
34 study miofascial pain syndrome: preliminary results *Histology and histopathology: cellular and molecular*
35 *biology* 30(S1):31-32
36
37 Sha JP, Heimur J 2012 New frontiers in the pathophysiology of myofascial pain *The pain practitioner* 22(2):26-
38 33
39
40 Sha, JP, Phillips TM, Danoff JV, Gerber LH 2005 An in vivo microanalytical technique for measuring the local
41 biochemical milieu of human skeletal muscle *Appl Physiol.* 99:1977-1984
42
43 Shankar H, Reddy S 2012 Two- and three-dimensional ultrasound imaging to facilitate detection and targeting
44 of taut bands in myofascial pain syndrome *Pain Med.* 13(7):971-5 [http://dx.doi.org/10.1111/j.1526-](http://dx.doi.org/10.1111/j.1526-4637.2012.01411.x)
45 [4637.2012.01411.x](http://dx.doi.org/10.1111/j.1526-4637.2012.01411.x)
46
47 Sikdar S, Shah JP, Gilliams E, Gebreab T, Gerber LH 2008 Assessment of myofascial trigger points (MTrPs): a
48 new application of ultrasound imaging and vibration sonoelastography *Conf Proc IEEE Eng Med Biol Soc*
49
50 Sikdar S, Shah JP, Gebreab T, Yen RH, Gilliams E, Danoff J, Gerber LH 2009 Novel applications of ultrasound
51 technology to visualize and characterize myofascial trigger points and surrounding soft tissue *Arch Phys Med*
52 *Rehabil.* 90(11):1829-38 <http://dx.doi.org/10.1016/j.apmr.2009.04.015>
53
54 Simons DG 2004 Review of enigmatic MTrPs as a common cause of enigmatic musculoskeletal pain and
55 dysfunction *J Electromyogr Kinesiol.* 14(1):95-107
56
57 Simons DG 2008 New views of myofascial trigger points: etiology and diagnosis *Arch Phys Med Rehabil.*
58 89(1):157-9 <http://dx.doi.org/10.1016/j.apmr.2007.11.016>
59
60 Simons DG, Travell JG, Simons LS 1999 *Myofascial pain and dysfunction: the trigger point manual Volumen 1*
Upper half of the body 2nd ed. (Baltimore: Williams & Wilkins)
61
62 Sinkjaer T, Toft E, Larsen K, Andreassen S, Hansen HJ 1993 Non-reflex and reflex mediated ankle joint
63 stiffness in multiple sclerosis patients with spasticity *Muscle Nerve* 16(1):69-76

1
2
3 Smidt N, van der Windt DA, Assendelft WJ, Mourits AJ, Devillé WL, de Winter AF, Bouter LM 2002
4 Interobserver reproducibility of the assessment of severity of complaints, grip strength, and pressure pain
5 threshold in patients with lateral epicondylitis Arch Phys Med Rehabil. 83:1145-50
6

7 Stratford PW, Goldsmith CH 1997 Use of the standard error as a reliability index of interest: an applied example
8 using elbow flexor strength data Phys Ther. 77(7):745-50.
9

10 Thomas K, Shankar H 2013 Targeting myofascial taut bands by ultrasound Curr Pain Headache Rep. 17(7):349
11 <http://dx.doi.org/10.1007/s11916-013-0349-4>
12

13 Takla MK, Razek NM, Kattabei O, El-Lythy MA 2016 A comparison between different modes of real-time
14 sonoelastography in visualizing myofascial trigger points in low back muscles J Man Manip Ther. 24(5):253-
15 263

16 Tous-Fajardo J, Moras G, Rodríguez-Jiménez S, Usach R, Doutres DM, Maffiuletti NA 2010 Inter-rater
17 reliability of muscle contractile property measurements using non-invasive tensiomyography J Electromyogr
18 Kinesiol. 20(4):761-6 <http://dx.doi.org/10.1016/j.jelekin.2010.02.008>
19

20 Turo D, Otto P, Hossain M, Gebreab T, Armstrong K, Rosenberger WF, Shao H, Shah JP, Gerber LH, Sikdar S
21 2015 Novel use of ultrasound elastography to quantify muscle tissue changes after dry needling of myofascial
22 trigger points in patients with chronic myofascial Pain J Ultrasound Med. 34(12):2149-61
23 <http://dx.doi.org/10.7863/ultra.14.08033>
24

25 Vain A, Kums T, Erelaine J, Pääsuke M, Gapeyeva H 2015 Gastrocnemius muscle tone, elasticity, and stiffness
26 in association with postural control characteristics in young men Proceedings of the Estonian Academy of
27 Sciences

28 Van Deun B, Hobbelen JS, Cagnie B, Van Eetvelde B, Van Den Noortgate N, Cambier D 2016 Reproducible
29 measurements of muscle characteristics using the MyotonPRO device: comparison between individuals with
30 and without paratonia J Geriatr Phys Ther. 00:1-10 <http://dx.doi.org/10.1519/JPT.0000000000000119>
31

32 Veldi M, Vasar V, Vain A, Hion T, Kull M 2000 Computerized endopharyngeal myotonometry (CEM): a new
33 method to evaluate the tissue tone of the soft palate in patients with obstructive sleep apnoea syndrome J Sleep
34 Res. 9(3):279-84
35

36 Viir R, Laiho K, Kramarenko J, Mikkelsen M 2006 Repeatability of trapezius muscle tone assessment by a
37 myometric method J. Mech. Med. Biol. 6(2):215-228
38

39 Wang J 2017 An analysis on muscle tone and stiffness of posterior cervical region during sling and plinth on
40 static prone position J Phys Ther Sci. 29:1841–1843 <http://dx.doi.org/10.1589/jpts.29.1841>
41

42 Weir JP 2005 Quantifying test-retest reliability using the intraclass correlation coefficient and the SEM. J
43 Strength Cond Res. 19: 231-240. <https://dx.doi.org/10.1519/15184.1>
44

45 Wepler CH, Magnusson SP 2010 Increasing muscle extensibility: a matter of increasing length or modifying
46 sensation? Phys Ther. 90(3):438-49 <http://dx.doi.org/10.2522/ptj.20090012>
47

48 Zinder SM, Padua DA 2011 Reliability, validity, and precision of a handheld myometer for assessing in vivo
49 muscle stiffness J Sport Rehabil. 6:Technical Notes 1 <http://dx.doi.org/10.1123/jsr.2010-0051>
50
51
52
53
54
55
56
57
58
59
60

Table 1. Sample characteristics (n=50).

| | |
|------------------------------|-------------|
| Age (years) | 24.6 ±7.9 |
| Sex (male%) | 58% |
| Height (m) | 1.71±0.08 |
| Weight (kg) | 68.64±13.44 |
| Body Mass Index (BMI) | 21.12±7.82 |

Values are mean ± SD

Table 2. Comparisons of frequency, decrement and stiffness of the medial myofascial trigger point and its taut band of soleus muscle.

| Variable | Rater | Myofascial Tissue | Mean ± SD | Mean difference (95% CI) | P Value | Effect Size (d) |
|------------------|-------|-------------------|--------------|-------------------------------|---------|-----------------|
| Frequency | 2 | MTrP | 15.87±1.75 | -0.55 (-1.279 to 0.179) | 0.138 | 0.299 |
| | | TB | 16.42±1.92 | | | |
| | 3 | MTrP | 16.17±1.74 | -0.49 (-1.245 to 0.249) | 0.189 | 0.266 |
| | | TB | 16.67±2.01 | | | |
| Decrement | 2 | MTrP | 1.19±0.20 | 0.012 (-0.074 to 0.098) | 0.392 | 0.048 |
| | | TB | 1.18±0.22 | | | |
| | 3 | MTrP | 1.22±0.21 | 0.045 (-0.041 to 0.131) | 0.242 | 0.232 |
| | | TB | 1.17±0.22 | | | |
| Stiffness | 2 | MTrP | 304.84±48.77 | -23.72 (-43.981 to -3.459) | 0.022* | 0.465 |
| | | TB | 328.56±53.22 | | | |
| | 3 | MTrP | 305.52±50.21 | -23.40 (-44.971 to -1.829) | 0.034* | 0.431 |
| | | TB | 328.92±58.19 | | | |

Abbreviations: MTrP, medial myofascial trigger point of soleus muscle; TB, taut band of MTrP; SD, standard deviation; CI, confidence interval.

*P<0.05; †P<0.01; ‡P<0.001

Table 3. Inter-rater reliability of myofascial tissue myotonometry.

| Measurement | | ICC (95% CI) | SEM (SEM%) | MDD ₉₅ (MDD ₉₅ %) |
|-------------|------|---------------------|---------------|---|
| Frequency | MTrP | 0.87 (0.78 to 0.92) | 0.63 (3.93%) | 1.74 (10.89%) |
| | TB | 0.97 (0.95 to 0.98) | 0.35 (2.11%) | 0.97 (5.85%) |
| Decrement | MTrP | 0.86 (0.76 to 0.98) | 0.24 (20.38%) | 0.68 (56.48%) |
| | TB | 0.94 (0.89 to 0.97) | 0.17 (14.76%) | 0.48 (40.90%) |
| Stiffness | MTrP | 0.93 (0.88 to 0.96) | 13.01 (4.26%) | 36.07 (11.82%) |
| | TB | 0.95 (0.92 to 0.97) | 11.95 (3.64%) | 33.12 (10.08%) |

Abbreviations: MTrP, medial myofascial trigger point of soleus muscle; TB, taut band of MTP; ICC, intraclass correlation coefficient; CI, confidence interval; SEM, standard error of measurement; SEM%, SEM divided by the mean of all measurements from the two assessments and multiplied by 100%; MDD, minimal detectable change; MDD%, MDD divided by the mean of all measurements from the two assessments and multiplied by 100%.

Table 4. Correlation coefficients (r) and CIs between myotonometric measurements of the medial myofascial trigger point and its taut band.

| Variable | Frequency | | Decrement | | Stiffness | | |
|-----------|-----------|----|---|-------------------------|---|---|---|
| | MTrP | TB | MTrP | TB | MTrP | TB | |
| Frequency | MTrP | - | 0.86[‡] (0.70 to 1.00) | 0.19 (-0.09 to 0.48) | 0.17 (-0.12 to 0.46) | 0.91[‡] (0.78 to 1.00) | 0.83[‡] (0.67 to 0.99) |
| | TB | - | - | 0.15 (-0.14 to 0.43) | 0.10 (-0.19 to 0.38) | 0.79[‡] (0.61 to 0.97) | 0.95[‡] (0.86 to 1.00) |
| Decrement | MTrP | - | - | - | 0.81[‡] (0.63 to 0.98) | 0.23 (-0.05 to 0.51) | 0.16 (-0.13 to 0.44) |
| | TB | - | - | - | - | 0.16 (-0.13 to 0.45) | 0.17 (-0.11 to 0.46) |
| Stiffness | MTrP | - | - | - | - | - | 0.79[‡] (0.62 to 0.97) |
| | TB | - | - | - | - | - | - |

Abbreviations: MTrP, medial myofascial trigger point of soleus muscle; TB, taut band of MTrP.

*Significant correlation (P<0.05).

†Significant correlation (P<0.01).

‡Significant correlation (P<0.001).

Table 5. Correlation coefficients (r) and CIs between myotonometric measurements and isokinetic measurements.

| Variable | PT ₁₀ | AT ₁₀ | PT ₁₈₀ | AT ₁₈₀ | E ₂₀₀ | E _{Tol} | F _{Tol} | |
|-----------|------------------|-------------------------|-------------------------|-------------------------|-------------------------|------------------|------------------|-----------------|
| Frequency | MTrP | 0.36* | 0.42[†] | 0.40[†] | 0.43[†] | -0.16 | -0.03 | 0.12 |
| | | (0.08 to 0.63) | (0.15 to 0.68) | (0.13 to 0.66) | (0.17 to 0.69) | (-0.45 to 0.14) | (-0.33 to 0.27) | (-0.18 to 0.42) |
| | TB | 0.33* | 0.38[†] | 0.43[†] | 0.46[†] | -0.17 | -0.09 | 0.10 |
| | | (0.06 to 0.60) | (0.11 to 0.64) | (0.17 to 0.69) | (0.20 to 0.72) | (-0.47 to 0.12) | (-0.39 to 0.21) | (-0.40 to 0.20) |
| Decrement | MTrP | -0.27 | -0.31* | -0.16 | -0.15 | 0.11 | 0.33* | 0.20 |
| | | (-0.55 to 0.01) | (-0.58 to -0.03) | (-0.45 to 0.13) | (-0.43 to 0.14) | (-0.18 to 0.41) | (0.05 to 0.62) | (-0.09 to 0.50) |
| | TB | -0.31* | -0.29* | -0.18 | -0.18 | 0.10 | 0.29* | 0.15 |
| | | (-0.58 to -0.03) | (-0.56 to -0.01) | (-0.47 to 0.10) | (-0.46 to 0.11) | (-0.20 to 0.40) | (0.00 to 0.58) | (-0.45 to 0.15) |
| Stiffness | MTrP | 0.40[†] | 0.45[†] | 0.45[†] | 0.48* | -0.26 | -0.19 | 0.07 |
| | | (0.13 to 0.67) | (0.19 to 0.71) | (0.19 to 0.71) | (0.23 to 0.73) | (-0.55 to 0.03) | (-0.48 to 0.11) | (-0.37 to 0.23) |
| | TB | 0.35* | 0.42[†] | 0.43[†] | 0.45[†] | -0.18 | -0.14 | 0.05 |
| | | (0.08 to 0.63) | (0.16 to 0.68) | (0.17 to 0.69) | (0.19 to 0.71) | (-0.48 to 0.11) | (-0.44 to 0.16) | (-0.25 to 0.35) |

Abbreviations: MTrP, medial myofascial trigger point of soleus muscle; TB, taut band of MTrP; PT₁₀, peak torque at 10°/s; AT₁₀, average torque at 10°/s; PT₁₈₀, peak torque at 180°/s; AT₁₈₀, average torque at 180°/s; E₂₀₀, ankle angle corresponding to 200 N; E_{Tol}, ankle dorsiflexion tolerance angle; F_{Tol}, force required for E_{Tol}.

*Significant correlation ($P < 0.05$).

[†]Significant correlation ($P < 0.01$).

[‡]Significant correlation ($P < 0.001$).

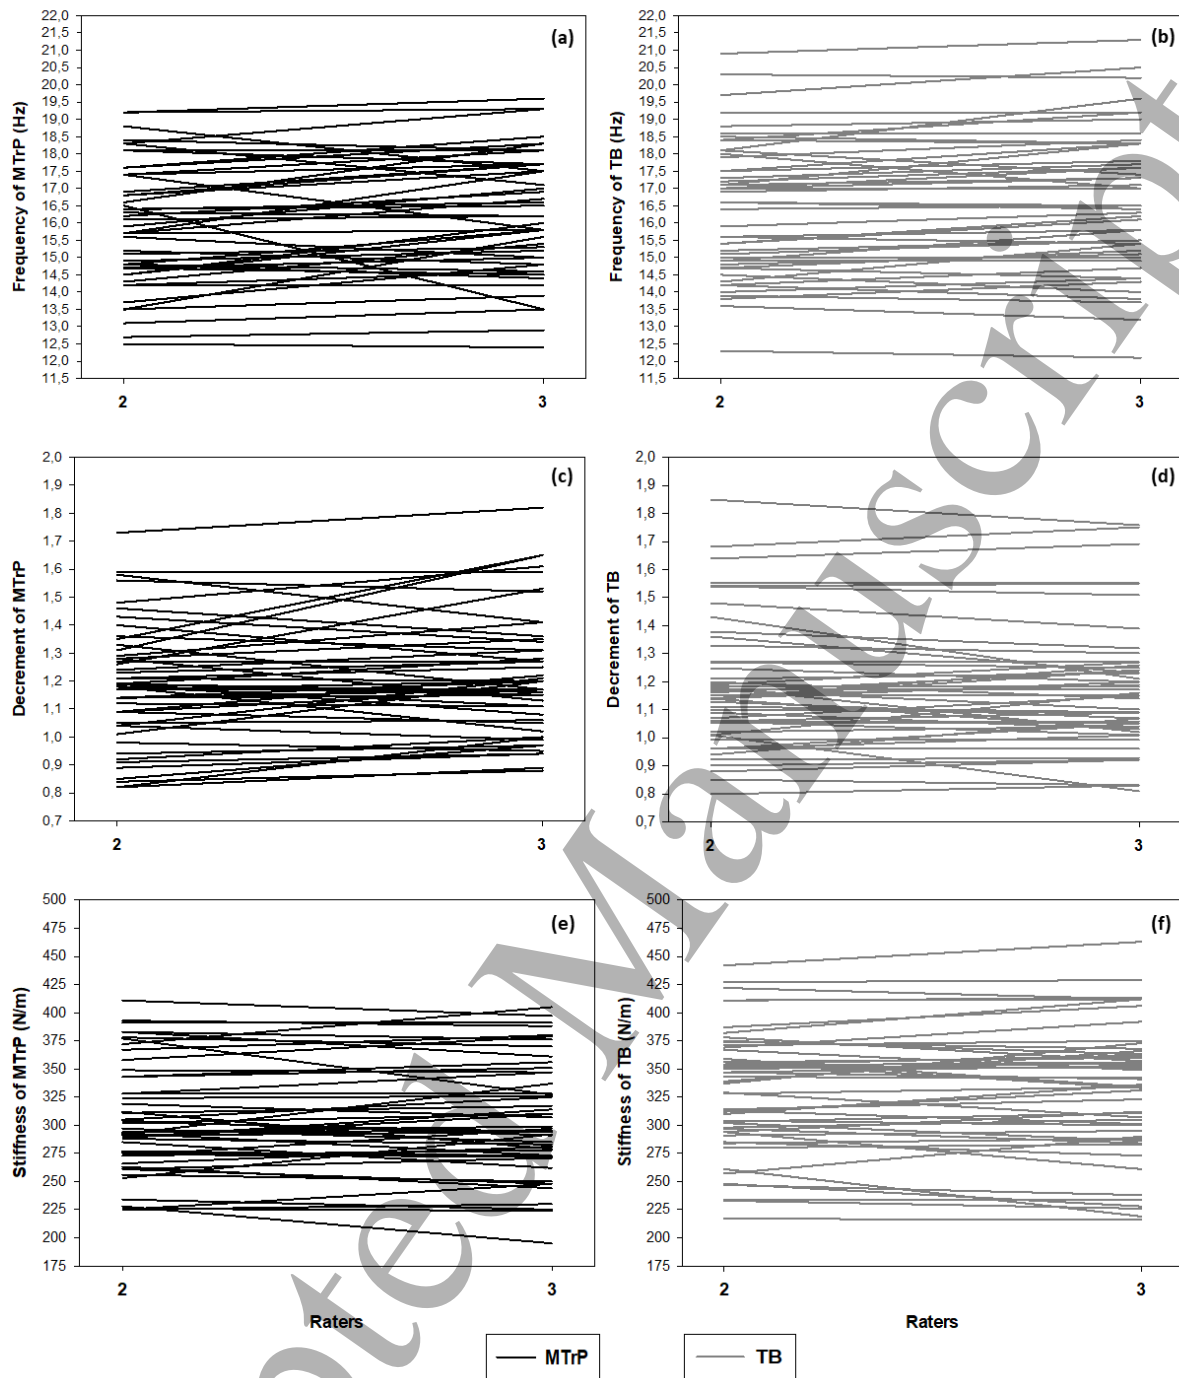


Figure 1. Individual subject profile ("Spaghetti") plots show the measurements from the two raters for each variable: (a) frequency of MTrP (Hz), (b) frequency of TB (Hz), (c) decrement of MTrP, (d) decrement of TB, (e) stiffness of MTrP (N/m) and (f) stiffness of TB (N/m). Abbreviations: MTrP, medial myofascial trigger point of soleus muscle; TB, taut band of MTrP.